


## Human IL-9 ELISA Ready-SET-Go!®

Catalog Number: 88-7958 Also Known As:Interleukin-9

RUO: For Research Use Only. Not for use in diagnostic procedures.

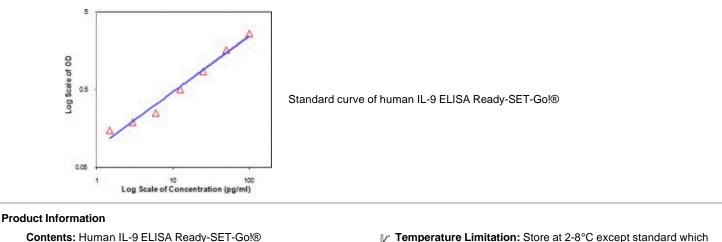

REF Catalog Number: 88-7958 Sensitivity: 1 pg/mL Standard Curve Range: 1-100 pg/mL Temperature Limitation: Store at 2-8°C except standard which should be stored at less than or equal to -70°C.
 Batch Code: Refer to Vial
 Use By: Refer to Vial
 Caution, contains Azide

#### Description

Interleukin-9 (IL-9) is a proinflammatory cytokine historically believed to be involved in type 2 immune responses. However, recent evidence suggests IL-9 may be secreted by a distinct T Helper lineage called Th9. These cells can either be derived from Th2 cells with TGF- $\beta$  or differentiated directly from naïve CD4+ T cells with TGF- $\beta$  and IL-4.

IL-9 is a member of the common cytokine receptor γ chain-dependent family of cytokines which also includes IL-2, IL-4, IL-7, IL-15 and IL-21. Its pleiotropic effects on Th2 lymphocytes, B lymphocytes, mast cells, eosinophils and gut and airway epithelial cells have implicated IL-9 in asthma and other allergy-related disorders.

This human IL-9 ELISA Ready-SET-Go! reagent set (with or without high-affinity binding microwell plates) contains the necessary reagents, buffers and diluents for performing quantitative enzyme linked immunosorbent assays (ELISA). This ELISA reagent set is specifically engineered for accurate and precise measurement of human IL-9 protein levels from samples including serum, plasma, and supernatants from cell cultures. The assay demonstrates parallelism in measuring recombinant and native human IL-9 proteins with a standard curve range of 1 pg/ml to 100 pg/ml.

Note: Please use eBioscience Cat. No. 39-8959 as ELISA standard if need additional vial of standard. eBioscience Cat. No. 14-8958 is not suitable for ELISA.

#### Components

Capture Antibody. Pre-titrated, purified antibody Detection Antibody. Pre-titrated, biotin-conjugated antibody Standard. Recombinant cytokine for generating standard curve and calibrating samples ELISA/ELISPOT Coating Buffer Powder. This Ready-Set-Go! ELISA Set may contain ELISA/ELISPOT Coating Buffer Powder (Reconstitute to 1L with dH20 and filter (0.22 uM)) or 10X PBS ELISA Coating Buffer (Dilute 1 part 10X Buffer into 9 parts dH20). Assay Diluent. 5X concentrated Detection enzyme. Pre-titrated Avidin-HRP Substrate Solution. Tetramethylbenzidine (TMB) Substrate Solution Certificate of Analysis. Lot-specific instructions for dilution of antibodies and standards 96 Well Plate. Corning Costar 9018 plates (included with product Cat. #'s ending in suffixes -22, -44, -76, -86)

#### **Applications Reported**

Human IL-9 ELISA Ready-SET-Go! has been reported for use in ELISA.

#### References

Veldhoen M, Uyttenhove C, van Snick J, Helmby H, Westendorf A, Buer J, Martin B, Wilhelm C, Stockinger B. Transforming growth factor-beta 'reprograms' the differentiation of T helper 2 cells and promotes an interleukin 9-producing subset. Nat Immunol. 2008 Dec;9(12):1341-6. Epub 2008 Oct 19.

Matsuzawa S, Sakashita K, Kinoshita T, Ito S, Yamashita T, Koike K. IL-9 enhances the growth of human mast cell progenitors under stimulation with stem cell factor. J Immunol. 2003 Apr 1;170(7):3461-7.

Nicolaides NC, Holroyd KJ, Ewart SL, Eleff SM, Kiser MB, Dragwa CR, Sullivan CD, Grasso L, Zhang LY, Messler CJ, Zhou T, Kleeberger SR, Buetow KH, Levitt RC. Interleukin 9: a candidate gene for asthma. Proc Natl Acad Sci U S A. 1997 Nov 25;94(24):13175-80.

Kelleher K, Bean K, Clark SC, Leung WY, Yang-Feng TL, Chen JW, Lin PF, Luo W, Yang YC. Human interleukin-9: genomic sequence, chromosomal location, and sequences essential for its expression in human T-cell leukemia virus (HTLV)-I-transformed human T cells. Blood. 1991 Apr 1;77(7):1436-41.

#### **Related Products**

39-8959 Human IL-9 Single-Use ELISA RSG Standard

Not for further distribution without written consent. Copyright © 2000-2012 eBioscience, Inc. Tel: 888.999.1371 or 858.642.2058 • Fax: 858.642.2046 • www.eBioscience.com • info@eBioscience.com



# Enzyme Linked Immunosorbent Assay (ELISA)

## **Research Use Only**

## Protocol: ELISA Ready-Set-Go!

The following protocol is a general guideline for the Ready-SET-Go! Sets

## **Materials Provided**

Please refer to the Certificate of Analysis (C of A) for components

## **Other Materials Needed**

- Buffers\*
  - Wash Buffer: 1x PBS, 0.05% Tween-20 (or eBioscience ELISA Wash Buffer Powder, Cat. No. 00-0400)
  - Stop Solution: 1M H<sub>3</sub>PO<sub>4</sub> (recommended) or 2N H<sub>2</sub>SO<sub>4</sub>
  - Pipettes
- Refrigerator & frost-free -20°C freezer
- 96-well plate (Corning Costar 9018 or NUNC Maxisorp<sup>®</sup>)
  NOTE: The use of ELISA plates which are not high affinity protein binding plates will result in suboptimal performance, e.g., low signal or inconsistent data. Do not use tissue culture plates or low protein absorption plates. Use only the Corning Costar 9018 or NUNC Maxisorp (Cat. No. 44-2404) 96-well plates
- 96-well ELISA plate reader (microplate spectrophotometer)
- ELISA plate washer (highly recommended)

NOTE: To ensure optimal results from this ELISA Ready-SET-Go! Set, please only use the components included in the set. Exchanging of components is not recommended as a change in signal may occur.

### **Time Requirements**

- 1 overnight incubation
- 4½-hour incubations
- 1 hour washing and analyzing samples

## Experimental Procedure

- Coat Corning Costar 9018 (or Nunc Maxisorp<sup>®</sup>) ELISA plate with 100 μL/well of capture antibody in Coating Buffer (dilute as noted on C of A, which is included with the reagent set). Seal the plate and incubate overnight at 4°C.
- Aspirate wells and wash 3 times with >250 μL/well Wash Buffer\*. Allowing time for soaking (~ 1 minute) during each wash step increases the effectiveness of the washes. Blot plate on absorbent paper to remove any residual buffer.
- Dilute 1 part 5X concentrated Assay Diluent with 4 parts DI water.\* Block wells with 200 μL/well of 1X Assay Diluent. Incubate at room temperature for 1 hour.
- 4. Optional: Aspirate and wash at least once with Wash Buffer.
- Using 1X Assay Diluent\*, dilute standards as noted on the C of A to prepare the top concentration of the standard. Add 100 µL/well of top standard concentration to the appropriate



## Enzyme Linked Immunosorbent Assay (ELISA) Research Use Only

wells. Perform 2-fold serial dilutions of the top standards to make the standard curve for a total of 8 points. Add 100  $\mu$ L/well of your samples to the appropriate wells. Seal the plate and incubate at room temperature for 2 hours (or overnight at 4°C for maximal sensitivity).

- 6. Aspirate/wash as in step 2. Repeat for a total of 3-5 washes\*\*.
- Add 100 μL/well of detection antibody diluted in 1X Assay Diluent\* (dilute as noted on C of A). Seal the plate and incubate at room temperature for 1 hour.
- 8. Aspirate/wash as in step 2. Repeat for a total of 3-5 washes\*\*.
- Add 100 μL/well of Avidin-HRP\* diluted in 1X Assay Diluent (dilute as noted on C of A). Seal the plate and incubate at room temperature for 30 minutes.
- 10. Aspirate and wash as in step 2. In this wash step, soak wells in Wash Buffer\* for 1 to 2 minutes prior to aspiration. Repeat for a total of 5-7 washes\*\*.
- Add 100 μL/well of Substrate Solution to each well. Incubate plate at room temperature for 15 minutes.
- 12. Add 50 µL of Stop Solution to each well.
- 13. Read plate at 450 nm. If wavelength subtraction is available, subtract the values of 570 nm from those of 450 nm and analyze data.

### NOTES:

# \* Be certain that no sodium azide is present in the solutions used in this assay, as this inhibits HRP enzyme activity.

\*\*The number of washes in the protocol was adapted to an automatic plate washer. This can be decreased when using other methods but should be tested empirically. Allowing time for soaking (~ 1 minute) during each wash step increases the effectiveness of the washes.



# Enzyme Linked Immunosorbent Assay (ELISA)

**Research Use Only** 

## **Quick Guide: Standard Calibration**

The following table indicates the protein standard contained in the Ready-SET-Go! is calibrated against NIBSC standards.

Table of Standard Calibration					
Cytokine	ng of eB standard	ng of NIBSC standard	U of NIBSC standard	NIBSC Lot #	
hIL-2	1	1.1	14.6	86/564	
hIL-4	1	2.2	22	88/656	
hIL-5	1	2.2	22	90/586	
hIL-6	1	1.7	170	89/548	
hIL-8	1	1.8	180	89/520	
hIL-10	1	0.8	4	93/722	
hIL-12	1	0.8	8	95/544	
hIL-17A	1	0.9	9000	01/420	
hIFN-g	1	1.1	22	87/586	
hTNF-a	1	0.9	36	87/650	
mIL-2	1	3.1	310	93/566	
mIL-4	1	3	30	91/656	
mIL-6	1	8.5	850	93/730	
mIFN-g*	1		4.5	Gg02-901-533	
mTNF-a	1	1.7	340	88/532	

\* Mouse IFN-g is calibrated using NIH standard (Lot Gg02-901-533) and is measured in Units (U)

ELISA Troubleshooting Guide				
Problem	Possibility	Solution		
A. High background	1. Improper and inefficient washing	1. Improve efficiency of washing. Fill plates completely, soak for 1 minute per wash, as directed		
	2. Cross contamination from other specimens or positive control	2. Repeat ELISA being careful when washing and pipetting		
	3. Contaminated substrate	3. Substrate should be colorless. Replace		
	4. Incorrect dilutions, e.g., conjugate concentration was too high	4. Repeat using correct dilutions		
B. No signal	1. Improper, low protein binding capacity plates were used	1. Repeat ELISA using recommended high binding capacity plates		
	2. Wrong substrate was used	2. Repeat ELISA using the correct substrate		
	3. Enzyme inhibitor present in buffers; e.g., sodium azide in the washing buffer and Assay Diluent inhibits peroxidase activity	3. Repeat ELISA making no enzyme inhibitor is present in any buffers.		

Not for further distribution without written consent. Copyright © 2000-2012 eBioscience, Inc. Tel: 888.999.1371 or 858.642.2058 • Fax: 858.642.2046 • www.ebioscience.com • info@ebioscience.com



# Enzyme Linked Immunosorbent Assay (ELISA)

# Research Use Only

	4. Coated capture antibody in Assay Diluent rather than Coating Buffer	4. Repeat ELISA using Coating Buffer contained in the set as the diluent for the capture antibody.
C. Very weak signal	1. Improper and inefficient washing	1. Make sure washing procedure is done correctly, with a soak time.
	2. Incorrect dilutions of standard	2. Follow recommendations of standard preparation exactly as written on the C of A
	3. Insufficient incubation time	3. Repeat ELISA following the protocol carefully for each step
	4. Incorrect storage of reagents	4. Store reagents at the correct temperature asn indicated on the Technical Data Sheet. Freezing certain components will severely impact results. Do not re-use the standards.
	5. Wrong filter in ELISA reader was used	5. Use the correct wavelength setting
	6. Wrong plate used	6. Use the recommended Corning Costar 9018 or NUNC Maxisorp flat bottom 96 well plates
D. Variation amongst replicates	1. Improper and inefficient washing	1. Make sure washing procedure is done correctly; see C of A. Edge effects can be avoided by moving samples and standards in from the edge of the plate.
	2. Poor mixing of samples	2. Mix samples and reagents gently and equilibrate to proper temperature
	3. Plates not clean	3. Plates should be wiped on bottom before measuring absorbance
	4. Reagents have expired	4. Order a new Ready-Set-Go ELISA.